



KONICA MINOLTA

Compatible with PWM-controlled sources

Illuminance Meter **T-10A** series

*Illuminance meters that conform to JIS AA Class and DIN Class B requirements.
Compatible with new, next-generation light sources including PWM-controlled sources*



Can be used for simple, inexpensive multi-point measurements. Mini receptor model also available to enable illuminance measurements even in narrow spaces.

For simple but accurate illuminance measurements. Makes creating illuminance measurement systems such as multi-point measurement systems easy!

Reliable, worry-free illuminance meters that conform to JIS AA Class and DIN Class B

Illuminance Meters T-10A and T-10MA conform to Class AA of JIS C 1609-1: 2006 "Illuminance meters Part 1: General measuring instruments" and DIN 5032 Part 7 Class-B "Photometry; classification of illuminance meters and luminance meters" requirements to provide high-accuracy, high-reliability, worry-free measurements.

Illuminance meters conforming to these standards are required for measurements of general illumination light sources, white LED lamps for illumination, etc. in a variety of industrial fields.

Removable receptor

The receptor and main body can be detached from each other and then connected using a LAN cable, making it easy to install as part of an inspection system.

Compatible with PWM-controlled lighting. Enables measurements of next-generation light sources.

Conventional illuminance meters often cannot accurately measure PWM-controlled light sources, but the T-10A series of illuminance meters can be used to accurately measure even such light sources.


Easy, inexpensive multi-point measurement (2 to 30 points).

Illuminance distribution of a projector etc. can be easily measured with a single instrument and several receptors.




Multi-point illuminance measuring system


● 5-point example: Architectural lighting, etc.

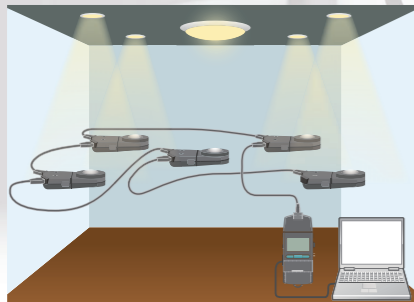

● 9-point example: Projectors, etc.

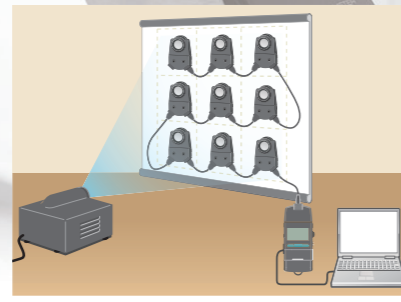


● 25-point example: Street lighting, etc.

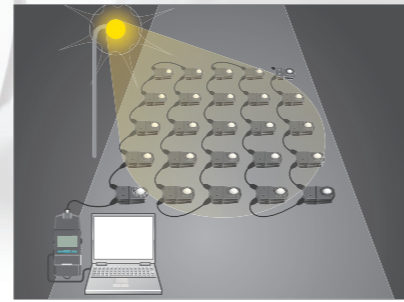


[T-10A 9-point measuring system composition]

Illuminance Meter T-10A	1 unit
T-10A Receptor head	8 units
Adapter units for Main Body T-A20	1 unit
Adapter units for Receptor Head T-A21	9 units
AC Adapter	1 unit
Data Management Software T-S10w	1 set


Main applications

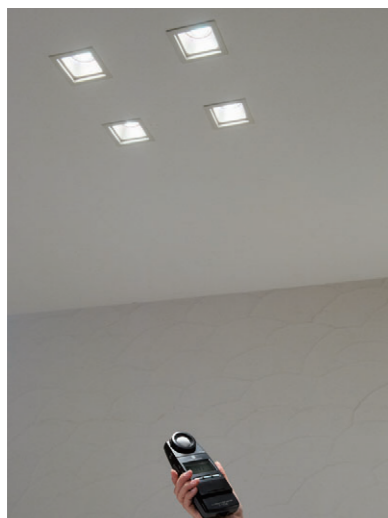

- Government testing organizations
- Research/inspection at illumination equipment makers
- Maintenance at factories, offices, hospitals, etc.

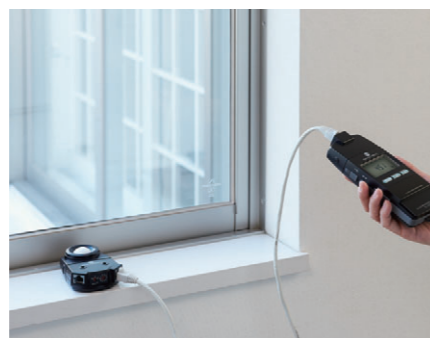

- Illuminance control of security lighting, street lighting, etc.
- As sensor for equipment measuring light-distribution characteristics, etc.

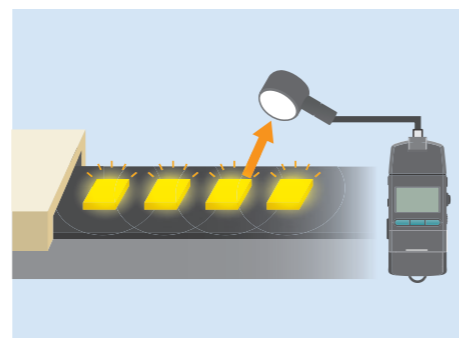

< Standard receptor >

T-10A



Receptor diffuser window: Ø 25 mm

T-10A

Conforms to JIS AA Class and DIN class B

Can be used for general measurements of illuminance.

< Mini receptor >

T-10MA/T-10W_sA/T-10W_LA



Receptor diffuser window: Ø 14 mm

T-10MA (Cord length: 1 m)

Conforms to JIS AA Class and DIN class B

Enables illuminance measurements of small areas.

Can be used for illuminance measurements in narrow spaces where the standard receptor won't fit. It can also be easily installed on various kinds of equipment or jigs for measuring light levels such as illumination.

T-10W_sA (Cord length: 5 m)


T-10W_LA (Cord length: 10 m)

Conforms to JIS requirements for special illuminance meters

Waterproof

Custom order

The mini receptor and cord are both waterproof, so they can be used for measurements in water. They can be used for illuminance control for fishery-related applications (such as fish farming, etc.) or for measuring outdoor illuminance on rainy days.

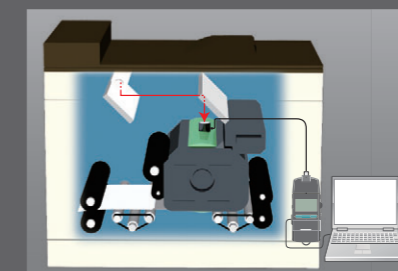

multi-point measurement systems easy!


Data Management Software T-S10w (Optional accessory)

Convenient, easy-to-use Excel® add-in software


Reads measurement data from T-10A series Illuminance Meters directly into Excel®. Further processing of data can then be performed easily using the various functions of Excel®.

Main specifications of Data Management Software T-S10w

Type	Add-in for Excel® (Excel® is required to use this add-in.)
Operating environment	One of the following environments with Excel®: Windows® 7 Professional 32-bit + Excel® 2007 32-bit or Excel® 2010 32-bit Windows® 7 Professional 64-bit + Excel® 2007 32-bit or Excel® 2010 32-bit Windows® 8.1 Pro 32-bit + Excel® 2010 32-bit or Excel® 2013 32-bit Windows® 8.1 Pro 64-bit + Excel® 2010 32-bit or Excel® 2013 32-bit Windows® 10 Pro 32-bit + Excel® 2013 32-bit or Excel® 2016 32-bit Windows® 10 Pro 64-bit + Excel® 2013 32-bit or Excel® 2016 32-bit *OS languages: English, Japanese, Simplified Chinese, Traditional Chinese *For details on system requirements for above versions of Windows® and/or Excel®, refer to their respective specifications. *Not compatible with 64-bit versions of Excel®.
Compatible instruments	T-10A, T-10MA, T-10WsA, T-10WLA, T-10, T-10M, T-10Ws, T-10WL

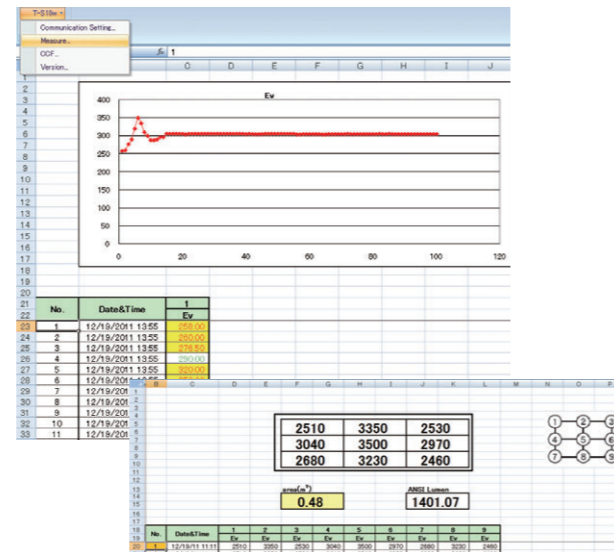

Relative Spectral Responsivity

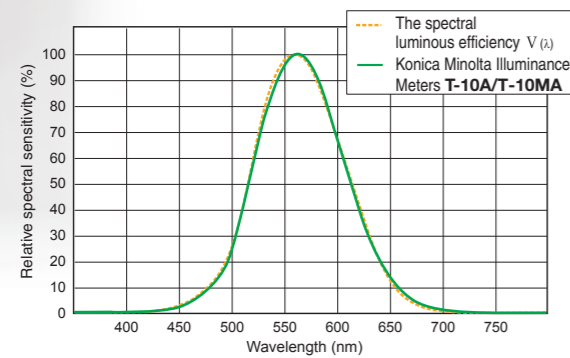


Ideally, the relative spectral responsivity of the illuminance meter should match $V(\lambda)$ of the human eye for photopic vision. As shown in the graph above, the relative spectral responsivity of Konica Minolta Illuminance Meters T-10A/10MA is within 6% ($f1'$) of the CIE spectral luminous efficiency $V(\lambda)$.

CIE; Commission Internationale de l'Éclairage

$f1'$ (CIE symbol); The degree to which the relative spectral responsivity matches $V(\lambda)$ is characterized by means of the error $f1'$.

Cosine Correction Characteristics

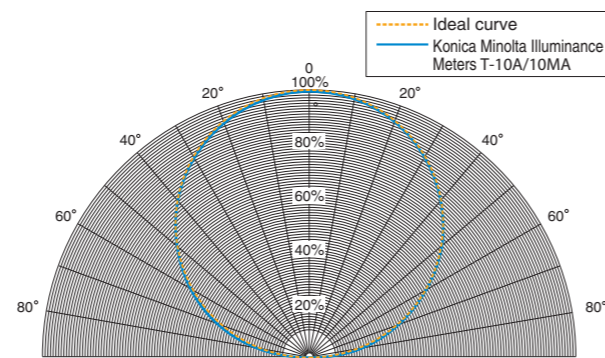


Since the brightness at the measurement plane is proportional to the cosine of the angle at which the light is incident, the response of the receptor must also be proportional to the cosine of the incidence angle. For Konica Minolta Illuminance Meters T-10A/10MA, the cosine response $f2$ is within 3%. The graph above shows the cosine correction characteristics of Konica Minolta Illuminance Meters T-10A/10MA.

About PWM-controlled lighting

PWM is the abbreviation of Pulse Width Modulation, and refers to the method of controlling signal intensity by controlling the ratio between the ON period and OFF period of a pulse signal.

A pulse signal is a signal which repeatedly alternates between ON and OFF, and the percentage of ON period during a single cycle is referred to as the "duty cycle".


PWM-controlled lighting is a method for controlling the brightness of a lamp by controlling the duty cycle (lit time) of light from a pulse-emission source. As the lit time becomes longer, the light becomes brighter, and conversely, as the lit time becomes shorter the light becomes darker.

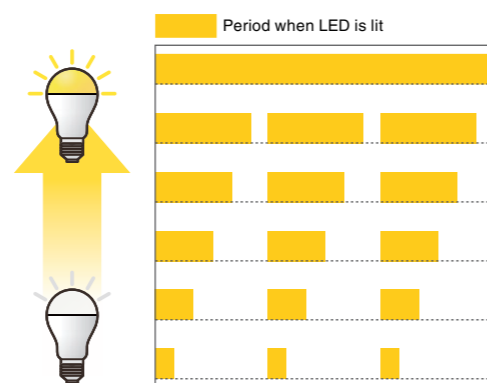

Konica Minolta's Illuminance Measurement Trio

Konica Minolta's line of instruments for measuring illuminance includes not only the Illuminance Meter T-10A which can measure PWM-controlled light sources, but also the Chroma Meter CL-200A which can measure color temperature and the Illuminance Spectrophotometer CL-500A which can measure color-rendering properties.

Illuminance meter that can handle PWM-controlled lighting

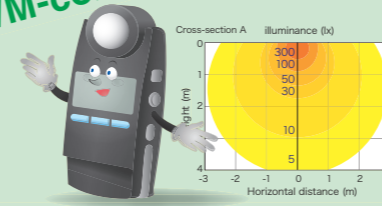


Illuminance Meter T-10A

Conforms to DIN Class B and JIS AA Class.

Capable of accurately measuring next-generation lamps including PWM-controlled lighting.

Multiple receptors can be used for easy, low-priced, multi-point measurement, and a miniature receptor model is also available for easily measuring illuminance in narrow spaces.

Measures color temperature

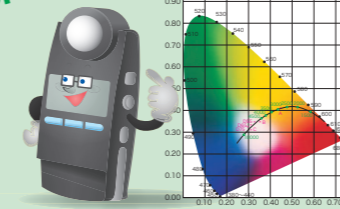


Chroma Meter CL-200A

A de facto industry standard for color-temperature measurement. Can also perform illuminance measurements (JIS AA Class).

Compact and lightweight with removable receptor connectable with extension cables.

Includes simple, convenient PC software as standard accessory.

Measures color-rendering properties

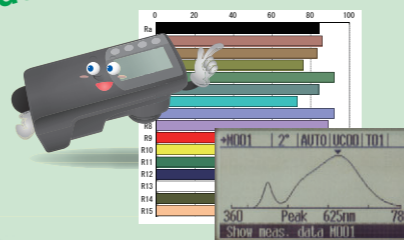

Illuminance Spectrophotometer CL-500A

The first illuminance spectrophotometer to conform to both JIS AA Class and DIN Class B requirements.

Compact, handheld type can easily be installed in inspection equipment and is ideal for evaluating color-rendering properties.

Includes simple, convenient PC software as a standard accessory.

* Both CL-200A and CL-500A can measure PWM-controlled lighting.

Illuminance-modified Spectroradiometer CS-2000A

Measurements of spectral irradiance are made possible by using the illuminance adapter. This makes it ideal for illuminance evaluation of projectors and LED or EL lighting.


This single instrument can be used for measuring both spectral radiance and spectral irradiance.

Our top-of-the-line CS-2000 is used for measuring various types of high-definition displays, and received the 13th Advanced Display of the Year 2008 Grand Prize in the Display Testing Equipment Category.

Spectral bandwidth: 5 nm or less (half bandwidth)
Measurable illuminance range:
1° measuring angle: 0.01 to 75,000 lx
0.1° measuring angle: 1.00 to 7,500,000 lx



System Diagram

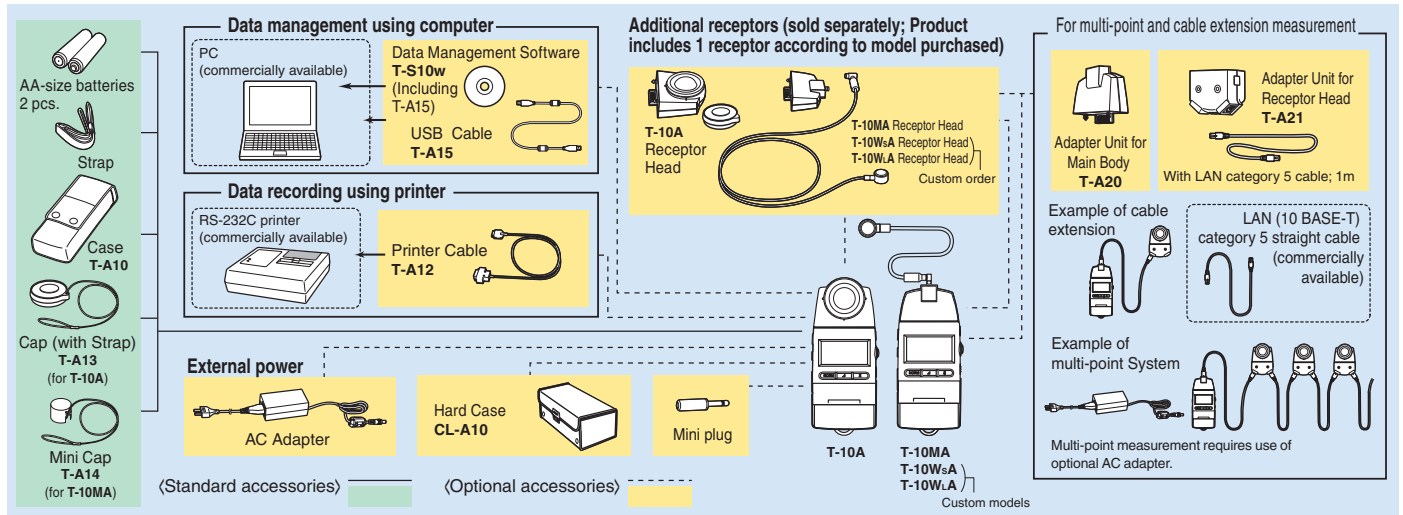

Main Specifications of T-10A

Model	Illuminance Meter T-10A (Standard receptor head)	Illuminance Meter T-10MA (Mini receptor head)	Illuminance Meter T-10W.sA (Waterproof mini receptor head)	Illuminance Meter T-10W.LA (Waterproof mini receptor head)
Type	Multi-function digital illuminance meter with detachable receptor head (Multi-point measurements of 2 to 30 points is possible)			
Illuminance meter class	Conforms to requirements for Class AA of JIS C 1609-1: 2006 "Illuminance meters Part 1: General measuring instruments" Conforms to DIN 5032 Part 7 Class B		Conforms to requirements for special Illuminance meters of JIS C 1609-1: 2006 *	
Receptor	Silicon photocell			
Relative spectral responsivity	Within 6% (f_1) of the CIE spectral luminous efficiency $V(\lambda)$			
Cosine correction characteristics (f_2)	Within 3%		Within 10%	
Measuring range	Auto range (5 manual ranges at the time of analog output)			
Measuring function	Illuminance (lx), illuminance difference (lx), illuminance ratio (%), integrated illuminance (lx-h), integration time (h), average illuminance (lx).			
Measuring range	Illuminance 0.01 to 299,900 lx; 0.001 to 29,990 fcd	Integrated illuminance 0.01 to 999,900 x 10 ³ lx-h	0.001 to 99,990 x 10 ³ fcd-h / 0.001 to 9999 h	1.00 to 299,900 lx; 0.1 to 29,990 fcd *2
User calibration function	CCF (Color Correction Factor) setting function: Measurement value x 0.500 to 2.000			
Linearity	$\pm 2\% \pm 1$ digit of displayed value			
Temperature/ humidity drift	Within $\pm 3\%$			
Measurement speed	2 times/sec. (continuous measurement with 1 receptor head)			
Computer interface	USB			
Printer output	RS-232C			
Analog output	1 mV/digit, 3 V at maximum reading; Output impedance: 10 K Ω ; 90% response time: 28 ms			
Display	3 or 4 Significant-digit LCD with backlight illumination (Automatic illumination)			
Power	2 AA-size batteries / AC adapter AC-A308 (optional; for 1 to 10 receptors) or AC adapter AC-A311 (optional; for 1 to 30 receptors)			
Battery performance	72 hours or longer (when alkaline batteries are used) in continuous measurement			
Operation temperature /humidity range	-10 to 40°C, relative humidity 85% or less (at 35°C) with no condensation		5 to 40°C, relative humidity of 85% or less (at 35°C) with no condensation	
Storage temperature / humidity range	-20 to 55°C, relative humidity 85% or less (at 35°C) with no condensation		0 to 55°C, relative humidity of 85% or less (at 35°C) with no condensation	
Size (W x D x H)	69 x 174 x 35 mm	Main body: 69 x 161.5 x 30 mm Receptor: $\varnothing 16.5$ x 13.8 mm		
Cord length	-	1 m	5 m	10 m
Weight (without battery)	200 g (7.0 oz.)	205 g	260 g (Receptor head only: 120 g)	340 g (Receptor head only: 200 g)

*1 Conforms to requirements for Class AA of JIS C 1609-1: 2006 for all items except cosine response (f_2).


*2 Although measurements below 1.00 lx are possible, they may not be stable due to the effects of electrical noise.

<Notes regarding mini receptors and waterproof mini receptors>

*Do not touch the cable during measurements. Doing so may result in unstable measurement values.

*Secure the cable during measurements. Failure to do so may result in unstable measurement values.

Dimensions (Units: mm)

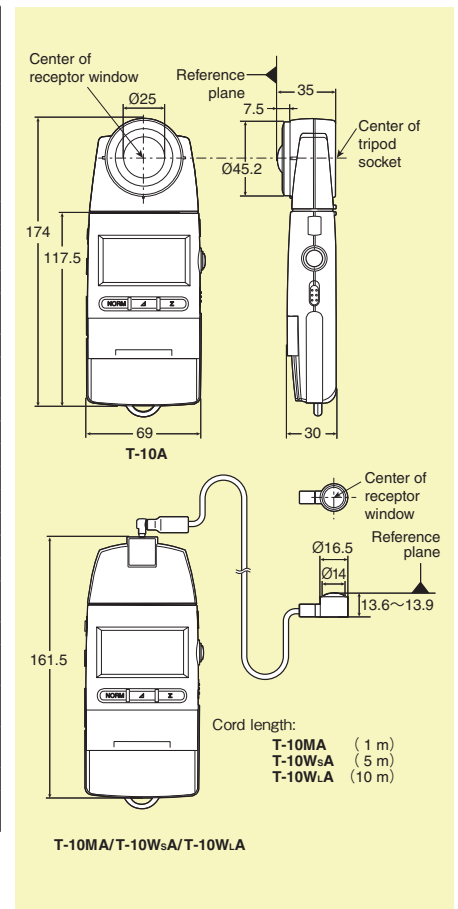

SAFETY PRECAUTIONS



For correct use and for your safety, be sure to read the instruction manual before using the instrument.

- Always connect the instrument to the specified power supply voltage. Improper connection may cause a fire or electric shock.

- Be sure to use the specified batteries. Using improper batteries may cause a fire or electric shock.

- KONICA MINOLTA, the Konica Minolta logo and symbol mark, and "Giving Shape to ideas" are registered trademarks or trademarks of KONICA MINOLTA, INC.
 - Windows® and Excel® are trademarks of Microsoft Corporation in the USA and other countries.
 - The specifications and appearance shown herein are subject to change without notice.
 - Screens shown are for illustration purpose only.
 - Some lamp control methods may make accurate measurements difficult.
- For details, please contact your nearest Konica Minolta sales office or dealer.

ISO Certifications of KONICA MINOLTA, Inc., Sakai Site



ISO 9001



ISO 14001

JQA-QMA15888
Design, development, manufacture/
manufacturing management, calibration, and
service of measuring instruments

JQA-E-80027
Design, development,
manufacture, service and sales
of measuring instruments

KONICA MINOLTA, INC.
Konica Minolta Sensing Americas, Inc.
Konica Minolta Sensing Europe B.V.

Osaka, Japan
New Jersey, U.S.A.
European Headquarter /BENELUX
German Office
French Office
UK Office
Italian Office
Swiss Office
Nordic Office
Polish Office
Turkish Office
SE Sales Division
Beijing Office
Guangzhou Office
Chongqing Office
Qingdao Office
Wuhan Office

Konica Minolta (CHINA) Investment Ltd.

Konica Minolta Sensing Singapore Pte Ltd.
Konica Minolta Sensing Korea Co., Ltd.

Addresses and telephone/fax numbers are subject to change without notice. For the latest contact information, please refer to the KONICA MINOLTA Worldwide Offices web page :

Phone : 888-473-2656 (in USA), 201-236-4300 (outside USA)
Nieuwegein, Netherlands **Phone** : +31 (0) 30 248-1193
München, Germany **Phone** : +49 (0) 89 4357 156 0
Roissy CDG, France **Phone** : +33 (0) 1 80 11 10 70
Warrington, United Kingdom **Phone** : +44 (0) 1925 467300
Cinisello Balsamo, Italy **Phone** : +39 02849488.00
Dietikon, Switzerland **Phone** : +41 (0) 43 322-9800
Västra Frölunda, Sweden **Phone** : +46 (0) 31 7099464
Wrocław, Poland **Phone** : +48 (0) 71 73452-11
Istanbul, Turkey **Phone** : +90 (0) 216-528 56 56
Shanghai, China **Phone** : +86 (0)21-5489 0202
Beijing, China **Phone** : +86 (0)10-8522 1551
Guangdong, China **Phone** : +86 (0)20-3826 4220
Chongqing, China **Phone** : +86 (0)23-6773 4988
Shandong, China **Phone** : +86 (0)532-8079 1871
Hubei, China **Phone** : +86 (0)27-8544 9942
Singapore **Phone** : +65 6563-5533
Goyang-si, Korea **Phone** : +82 (0) 2-523-9726

Fax : 201-785-2482
Fax : +31 (0) 30 24 81 211
Fax : +49 (0) 89 4357 156 99
Fax : +33 (0) 1 80 11 10 82
Fax : +44 (0) 1925 711143
Fax : +39 02849488.30
Fax : +41 (0) 43 322-9809

Fax : +48 (0)71 734 52 10
Fax : +90 (0) 212-253 49 69
Fax : +86 (0)21-5489 0005
Fax : +86 (0)10-8522 1241
Fax : +86 (0)20-3826 4223
Fax : +86 (0)23-6773 4799
Fax : +86 (0)532-8079 1873
Fax : +86 (0)27-8544 9991
Fax : +65 6560-9721
Fax : +82 (0)31-995-6511

<https://konicaminolta.com/instruments/network>

9242-4871-12 BJDPKI2